

Instruction sheet for new Check Valve



DESCRIPTION : Assembly for the new check valve on reagent tubing.

SCV67220-CHECK VALVE
Barb for 3/32" (2.4 mm) ID tubing SCV67220 x 3/32" (2.4 mm) ID tubing



Used in product: HG-302/HG-702

CAT. Part No : 970-110-8086



		DATE	NAME	SIG.
Work Check No.	REV.	APPROVED BY :	04/01/2016	Daniel Cohen Khallas
	A	SHEET 1 Of 2		



Cut the pipe with a cutter



Connect the Check Valve with the white connector facing downwards

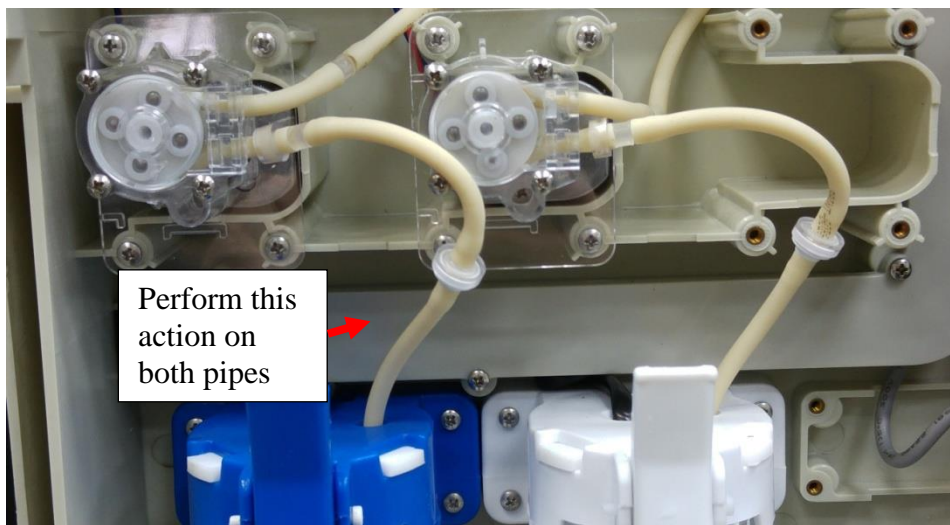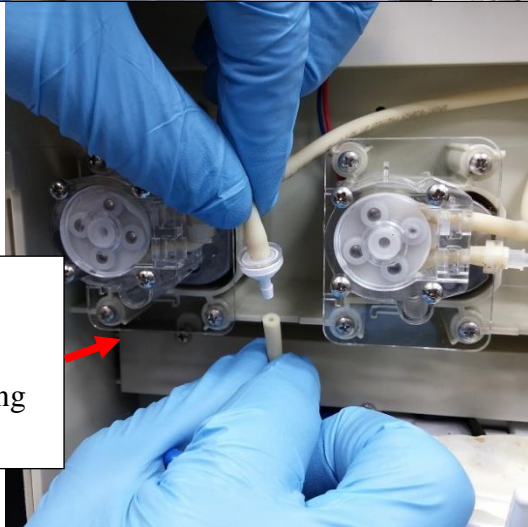

Perform this action on both pipes

****Note : In case you have a Free and Total Analyzer, you need to install a Check Valve also on the DPD3 tube.***